

TEST REPORT



No:200055441

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: XCNA-0204-44

ISSUE DATE:2020-04-11

扫码下载报告



SAMPLE INFORMATION:

TWENTY-FIVE KN95 MASKS

BRAND: SUREBLUE

COLOUR: WHITE

SIZE: 54001 54002 54002V 54003V 55001 55001V

DATE RECEIVED/DATE TEST STARTED: 2020-03-30

CONCLUSION:

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"—" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200055440.


ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).

COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.

THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:


Lian Liu ENGINEER



PAGE 1 OF 3

TEST REPORT

No: 200055441

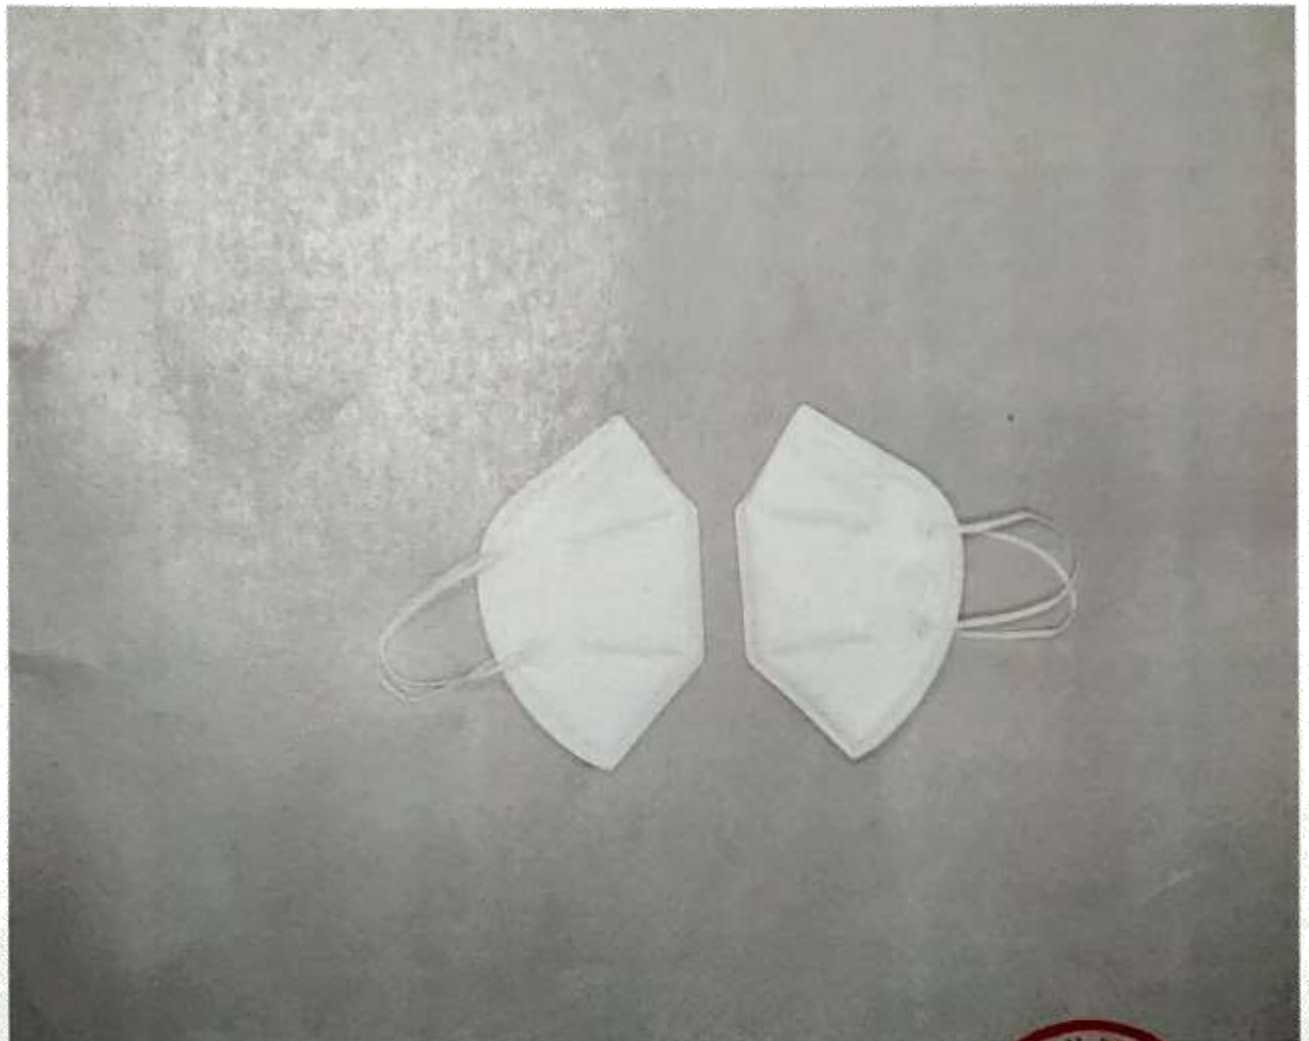

PAGE 2 OF 3

TEST REPORT

No: 200055441

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER

(GB 2626-2006 6.3, AIR FLOW: 85L/min, AEROSOL: NaCl, AEROSOL CONCENTRATION: 15mg/m³, TEMP: 23.2°C, RH: 36.2%)

FILTRATION EFFICIENCY (%):

UNTREATED SAMPLE

1# 98.70
2# 98.89
3# 98.57
4# 98.80
5# 99.011
6# 98.42
7# 98.55
8# 98.45
9# 98.68
10# 98.74

CONDITIONING TREATED

1# 97.75
2# 98.03
3# 97.80
4# 97.28
5# 97.54

REQUIREMENT

FILTRATION EFFICIENCY (%):

≥ 95.0
(KN95)
(GB 2626-2006)

INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 81.6
2# 83.3

PRETREATMENT SAMPLE:

1# 80.0
2# 79.4

REQUIREMENT

≤ 350
(GB 2626-2006)

EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 72.3
2# 73.2

PRETREATMENT SAMPLE:

1# 76.3
2# 74.5

REQUIREMENT

≤ 250
(GB 2626-2006)



—End of Report—

PAGE 3 OF 3